INSTRUCTIONS FOR USE
KLYGEFA™ (klahy-gef-uh)
(gefurulimab-gaks)
injection, for subcutaneous use
Single-dose prefilled autoinjector

This Instructions for Use contains information on how to inject KLYGEFA using the prefilled autoinjector.




Your healthcare provider should show you or your caregiver how to use the prefilled autoinjector the right way. If you or your caregiver have any questions, talk to your healthcare provider.

For subcutaneous injection only (inject directly under the skin).

Check your prescription

If you were prescribed:

600 mg
Use **2 prefilled autoinjectors** to give 2 injections.



Second injection is given immediately after the first injection.

or

300 mg
Use **1 prefilled autoinjector** to give 1 injection.



Your first dose is different from your weekly dose and will require 2 or 3 injections, depending on your body weight.

Unsure of your dose? Call your healthcare provider or pharmacist.

Important Information Before Injecting KLYGEFA

Storing KLYGEFA

- Store KLYGEFA in the refrigerator between 36°F to 46°F (2°C to 8°C) in the original carton to protect from light.
- KLYGEFA can be taken out of the refrigerator and placed back in the refrigerator 1 time, if needed. Do not keep KLYGEFA out of the refrigerator for more than 24 hours. Protect from light when stored at room temperature.
- Throw away (discard) the autoinjector if it has been left out at room temperature for more than 24 hours.
- Do not freeze KLYGEFA.
- Do not shake KLYGEFA.
- Do not expose KLYGEFA to heat.
- Keep KLYGEFA and all medicines out of the reach of children.

Handling KLYGEFA

- **Do not** remove needle cap until you are ready to inject to prevent the medicine from drying out.
- Grip the autoinjector body and keep hands away from the needle end to prevent a needle stick.
- **Do not** touch the purple needle end. This could cause the autoinjector to activate early.
- **Do not** re-cap as you may stick yourself or damage the needle.
- **Do not** use KLYGEFA if it has been previously used.
- **Do not** use KLYGEFA if it was dropped, damaged, or appears to be tampered with.


- **Do not** use KLYGEFA if it is past the expiration date (EXP).
- **Do not** use KLYGEFA if it contains particles.
- **Do not** use KLYGEFA if the needle has touched any surface after cap removal.

If any of these apply, throw away (dispose of) the autoinjector in a puncture-resistant sharps disposal container and use a new autoinjector.


KLYGEFA autoinjector

After the injection is complete, the purple needle end will lock in place over the needle.

Before use:

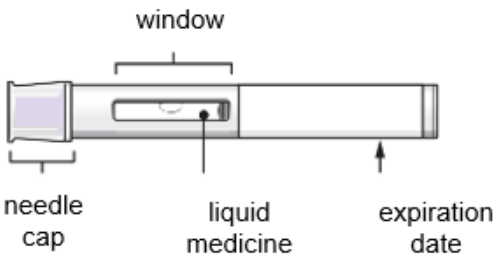

After use:

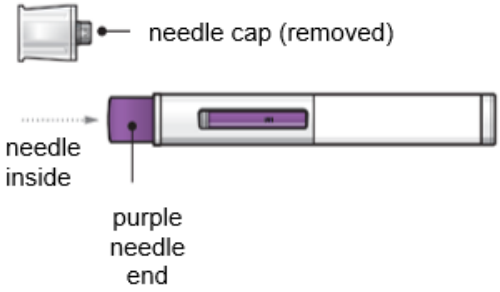

Prepare KLYGEFA


1. Confirm your dose

Check your prescription to confirm the dose your healthcare provider has prescribed.

If you were prescribed:

600 mg

Use **2 prefilled autoinjectors** to give 2 injections.



or

300 mg

Use **1 prefilled autoinjector** to give 1 injection.



Your first dose is different from your weekly dose and will require 2 or 3 injections, depending on your body weight.

2. Gather supplies

Gather the following supplies on a clean, flat workspace:

(See Figure A)

- Alcohol swabs
- Cotton balls
- Bandages
- Sharps disposal container

Note: Supplies listed are not included with autoinjector.



Figure A

3. Remove cartons needed from the refrigerator

Remove the number of cartons needed for your dose from the refrigerator. (See Figure B)

Inspect the cartons for any damage.

Check the expiration date.

4. Remove autoinjectors from the carton

Open the cartons.

Grip the autoinjector body and remove the autoinjector from the carton. (See Figure B)

Return extra autoinjectors back into the refrigerator in their carton.

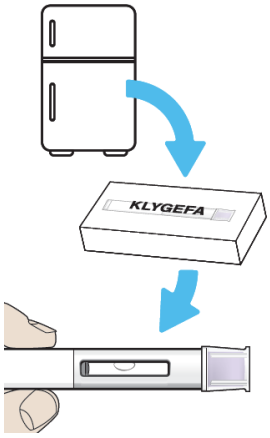


Figure B

5. Inspect autoinjector

Check the autoinjector for any damage.

Check the expiration date. (See Figure C)

- **Do not** touch the purple needle end. This may cause the autoinjector to activate early.
- **Do not** use if the expiration date has passed or there are signs of damage.




Figure C

6. Inspect medicine

Check the medicine to make sure the liquid is clear and slightly yellow to yellow.

(See Figure D)

Confirm there are no particles in the liquid. Do not use the autoinjector if the liquid is cloudy, discolored, or has flakes or particles in it.

It is normal to see air bubbles.

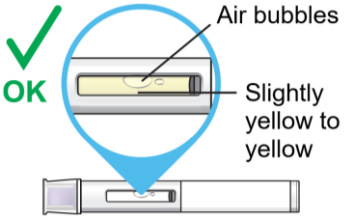


Figure D

7. Allow autoinjector to warm

Let the autoinjector sit at room temperature for 45 minutes before use. Protect from light. (See Figure E)

This will make the injection more comfortable.

- **Do not** use external heat sources such as a microwave or hot water to warm the autoinjector.
- **Do not** use the autoinjector if it has been out of the refrigerator for more than **24 hours** or previously frozen. Safely throw away (dispose of) the autoinjector and use a new one.



Figure E

8. Wash your hands

Wash your hands well with soap and water. (See Figure F)




Figure F

9. Choose injection site

Use a different injection site from your previous injection. If your prescribed dose requires more than 1 injection, leave a 1-inch (2.5 cm) space between injection sites. Do not inject into the exact same spot.

Choose from the following areas for your injection:

(See Figure G)

- Lower stomach area (lower abdomen), except the 2-inch (5 cm) area around your belly button (navel)
- Front of thighs
- Back of upper arms (injection by caregiver only)

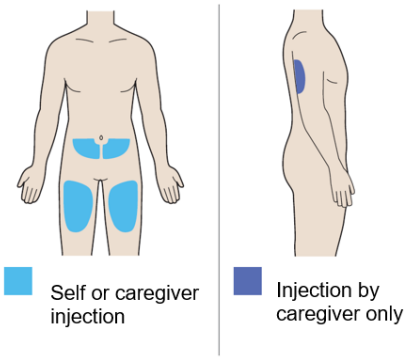


Figure G

10. Clean injection site

Clean any injection site with an alcohol swab and allow the skin to air dry. (See Figure H)

- **Do not** inject into itchy, hard, tender, painful, bruised, red or scarred skin.
- **Do not** touch the injection site again or blow on it before the injection.

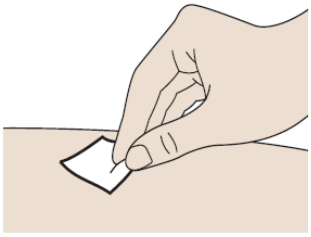


Figure H

Inject KLYGEFA

Things to know before you inject:

- **Do not** remove needle cap until you are ready to inject to prevent the medicine from drying out.
- **Do not** use the autoinjector if it has been dropped.
- **Do not** re-cap as you may stick yourself or damage the needle.
- **Do not** touch the purple needle end as this may cause the autoinjector to activate early.

11. Remove needle cap

Hold the autoinjector by its body and pull the needle cap straight off.

(See Figure I)

Throw away (dispose of) the needle cap right away.

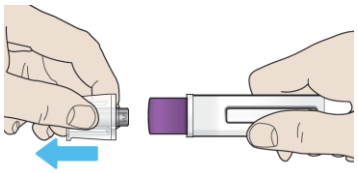


Figure I

12. Position the autoinjector

Grip the autoinjector firmly. Be careful not to cover the window.

Position the purple needle end flat against your skin with the window facing you. (See Figure J)


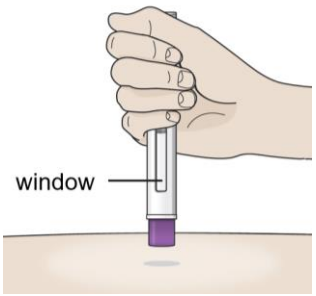


Figure J

13. Push down firmly

Push down to start the injection and hold firmly.

Count out loud slowly to 15, making sure you hold the autoinjector down to deliver all the medicine.

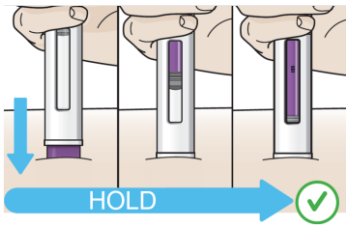

You may hear clicks before you get to 15 but keep holding the autoinjector down. (See Figure K)

Figure K

14. Confirm injection is complete

Before lifting the autoinjector up, make sure the window is all purple.

Then lift the autoinjector straight up. (See Figure L)


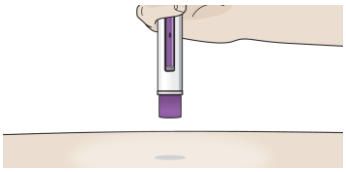


Figure L

If your dose is 600 mg
With a second autoinjector, repeat injection starting at step 5. Inject into a spot 1 inch away from first injection.

or

If your dose is 300 mg
Continue to step 15.



15. Check injection site

Check the injection site. If you see blood, press a cotton ball or gauze on the injection site. (See Figure M)

Apply a bandage if necessary. **Do not** rub the injection site.

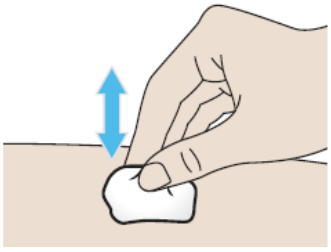


Figure M

Throw away (dispose of) KLYGEFA

16. Throw away (dispose of) used autoinjector

Put your used autoinjectors in an FDA-cleared sharps disposal container right away after injection. (See Figure N)

- **Do not** throw away your autoinjector in your household trash.

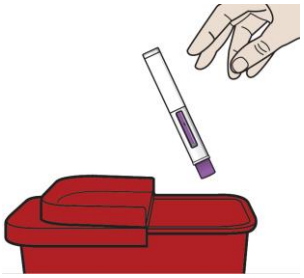


Figure N

If you do not have an FDA-cleared sharps disposal container, you may use a household container that is:

- made of a heavy-duty plastic,
- can be closed with a tight-fitting, puncture resistant lid, without sharps being able to come out,
- upright and stable during use,
- leak-resistant, and
- properly labeled to warn of hazardous waste inside the container.

When your sharps disposal container is almost full, you will need to follow your community guidelines for the correct way to dispose of your sharps disposal container.

There may be state or local laws about how you should throw away used needles and autoinjectors. For more information about safe sharps disposal, and for specific information about sharps disposal in the state that you live in, go to the FDA's website at: http://www.fda.gov/safesharpsdisposal

- **Do not** dispose of your used sharps disposal container in your household trash unless your community guidelines permit this.
- **Do not** recycle your used sharps disposal container.

Need help?

For additional assistance call 1-888-765-4747.

Frequently Asked Questions

Why do I need to allow the autoinjector to warm up at room temperature for 45 minutes prior to injecting?

- This step is primarily for your comfort. Never try to speed up the warming process in any way, like using the microwave or placing the autoinjector in warm water.

How many autoinjectors do I need for my prescribed dose?

- Check your prescription to confirm the dose your healthcare provider has prescribed. If you are prescribed a 600 mg dose, use 2 autoinjectors to administer the full dose. If you are prescribed a 300 mg dose, use 1 autoinjector to administer the full dose.

Can I perform my second injection in the same location?

- You can inject in the same area but leave 1 inch (2.5 cm) space between injection sites.

What if my autoinjector appears to be broken or damaged?

- Do not use the autoinjector. Contact your healthcare provider or pharmacist for further instructions.

What if I see air bubbles in my autoinjector?

- Air bubbles are normal.

What if my medicine is yellowish?

- The medicine is safe to use if the liquid is clear and slightly yellow to yellow.

Why do I need to hold the autoinjector down for 15 seconds during the injection?

- This is necessary to make sure that you receive the full dose.

Where should I dispose of the needle cap?

- You can dispose of the needle cap in your household trash.

Manufactured by:

Alexion Pharmaceuticals, Inc.
Boston, MA 02210 USA

U.S. License Number 1743

KLYGEFA is a trademark of Alexion Pharmaceuticals, Inc.

© 2026 Alexion Pharmaceuticals, Inc.

For more information, go to www.KLYGEFA.com or call 1-888-765-4747. If you still have questions, contact your healthcare provider.

This Instructions for Use has been approved by the U.S. Food and Drug Administration. Issued: 11/2026